

Installation Manual

NeoSoft, LLC



NS-03-028-0003 Rev 1
Copyright 2017 NeoSoft, LLC
All rights reserved

Manufacturer



NeoSoft, LLC
N27 W23910A Paul Road
Pewaukee, WI 53072 USA

Phone: 262-522-6120
website: www.neosoftllc.com

Sales: orders@neosoftmedical.com
Service: service@neosoftmedical.com

Table of Contents

suiteDXT Installation & Configuration **1**

- Prerequisites 1
- Installation 2
- Configuration 2
- Local Storage Tab 5
- Application Launch Tab 6
- Feature Licensing Tab 7
 - Request a License 8*
 - Apply the License 8*
- Tablet Mode 8

suiteHEART® Software Installation **9**

- Prerequisites 9
- Installation 10
- Application Inactivity Setting 10
- Licensing Schemes 10
 - Remote Connectivity 11*

This page intentionally left blank.

Medical device directive

This product conforms with the requirements of council directive 93/42/EEC concerning medical devices when it bears the following CE mark of Conformity:



European Representatives:



EMERGO EUROPE
Prinsessegracht 20
2514 AP The Hague
The Netherlands



CAUTION: *United States federal law restricts this device to sale by, or on the order of, a physician.*

This page intentionally left blank.

suiteDXT Installation & Configuration

Prerequisites

Prior to installation of the software, the following prerequisites must be met:

Table 1: System Requirements

Minimum System Requirements
Supported Operating Systems: <ul style="list-style-type: none">• Windows 7 Professional or Enterprise with SP1 (64 bit version)• Windows 10 Professional or Enterprise (64 bit version)
Video card (NVIDIA); 4GB RAM, minimum of 1664 CUDA Cores, support for OpenGL 4.0, support 1920 x 1080 resolution or higher
Monitor shall support 1920 x 1080 resolution or higher
Anti-Virus/Anti-Malware software installed
Minimum 16GB memory
Available hard drive space minimum 25GB
PDF viewer, Adobe Reader 11.0 or higher
An open network port for DICOM transfer over network
Static IP address (recommended)
CUDA Toolkit version 8.0.61 or later
Solid-State hard drive
Intel® Core™ i7 processor
27" Monitor

NOTE: In the event that the host system loses or is reassigned its IP address, remote devices will need to be manually reconfigured to request and accept network traffic.

NOTE: You must be logged into your operating system as Administrator in order to install the software, restart the DICOM service, and move the Local DICOM Storage.

Installation

1. Double click suiteDXT-windows-installer.
2. If prompted, select "Yes" on the User Account Control pop-up.
3. Select the desired language, then click "OK."

NOTE: If another version of the software is already installed on the system, a pop-up will ask permission to overwrite. Click "Yes" to continue with the installation.


4. Select "Next" on the suiteDXT setup screen.
5. Check the box for "I accept the agreement" and select "Next."
6. Accept or change the installation directory and select "Next."
7. Select "Next" in ready to install setup screen.
8. Select "Finish" in the setup screen.

Configuration

You will need to run through the configuration steps when suiteDXT is newly installed or when/if the static IP address is renewed.

1. Launch suiteDXT via the desktop shortcut or navigate through the start menu, Start > All Programs> suiteDXT> suiteDXT
If prompted, select "Yes" on the user account pop-up.
2. Select the Configuration button, outlined in the figure below.


FIGURE 1. suiteDXT Main Screen

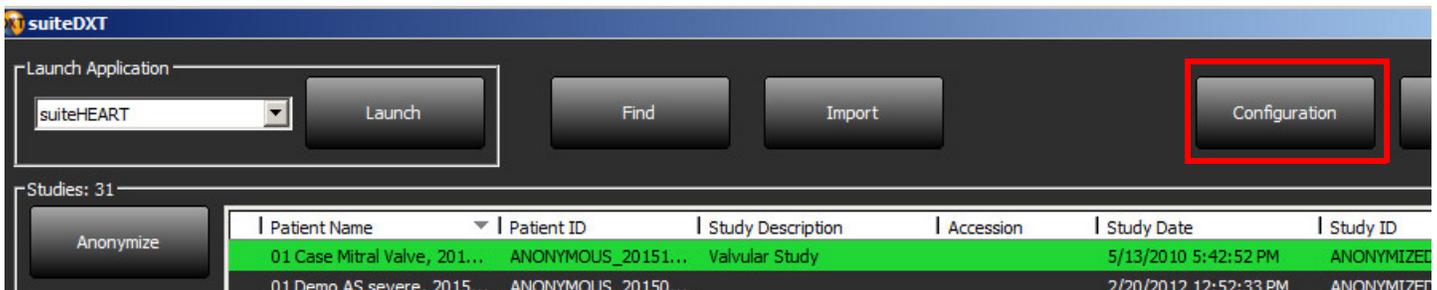

3. On the DICOM Configuration tab, enter information for the local host: (Figure 2)
 - Description (enter any descriptor of your choosing).
 - AE Title (case sensitive) is the name used to identify the host by other hosts.
 - Port (104).


NOTE: The information entered on this tab must be entered exactly the same on any remote device for suiteDXT to retrieve or accept images from the remote host.

FIGURE 2. Configuration Tab Window

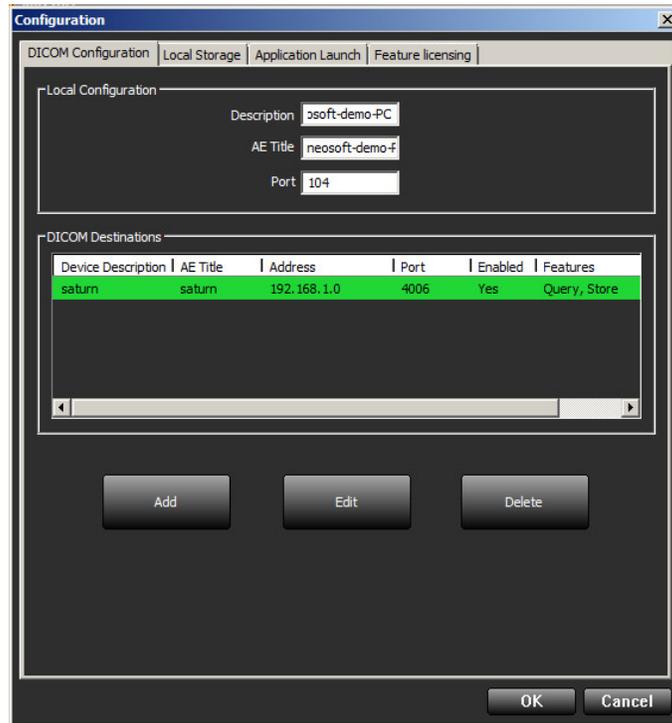


4. If available, perform a DICOM echo from any remote device to this host to ensure DICOM connectivity.
5. Select the “Add” button to input all DICOM destinations (remote hosts).
 - Description
 - AE Title
 - Address
 - Port
 - Select the checkboxes for: Enabled; Store to device and Query device (Figure 3).

FIGURE 3. DICOM Configuration Window

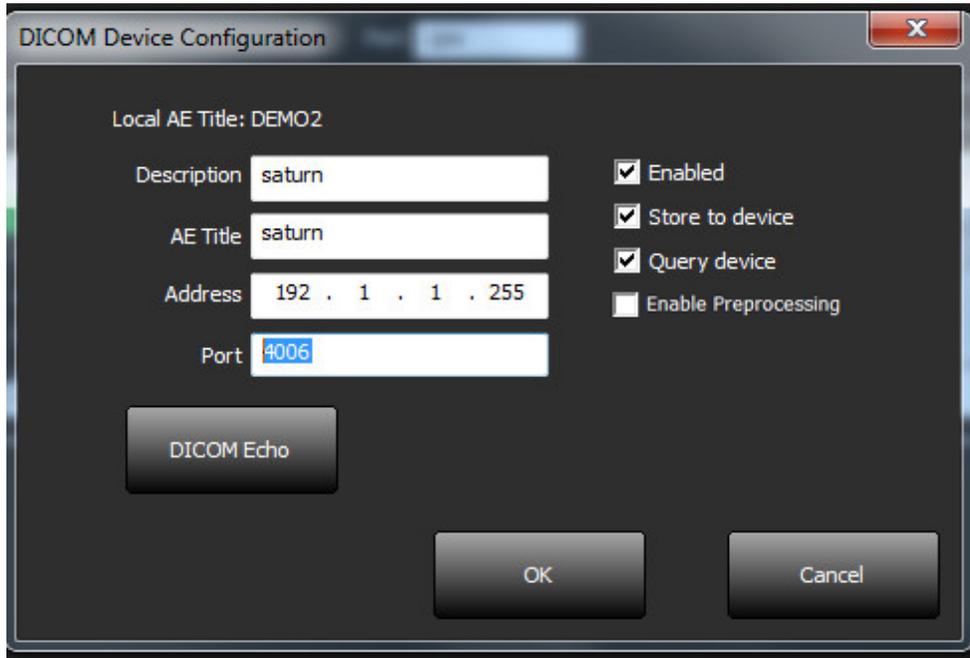

6. Select the “DICOM Echo” button.
 - If you don’t see the DICOM Success Message window (Figure 4) contact your network administrator.


FIGURE 4. DICOM Success Message

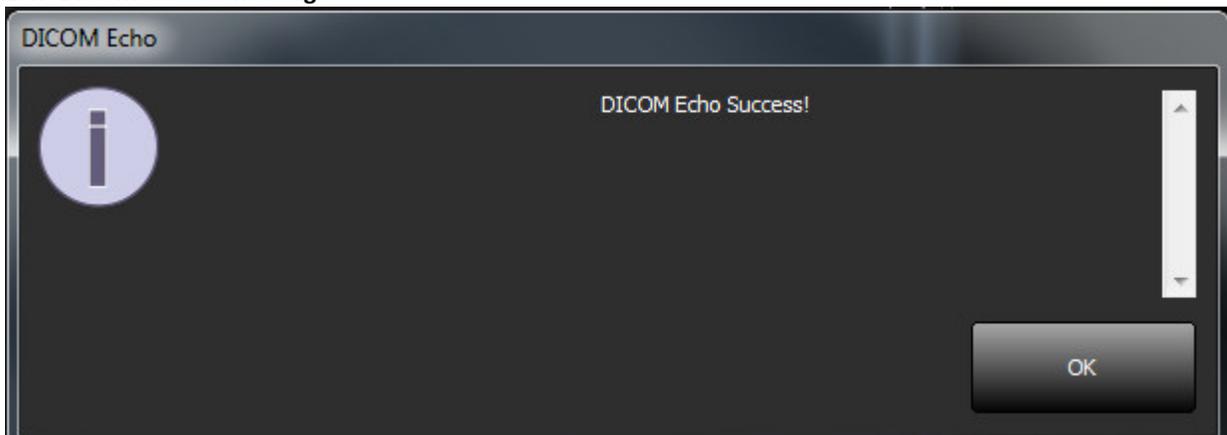

NOTE: DICOM Destinations can be modified and a DICOM echo performed via the Edit button and destinations can be deleted via the Delete button.

Local Storage Tab


FIGURE 5. Local Storage Tab Window

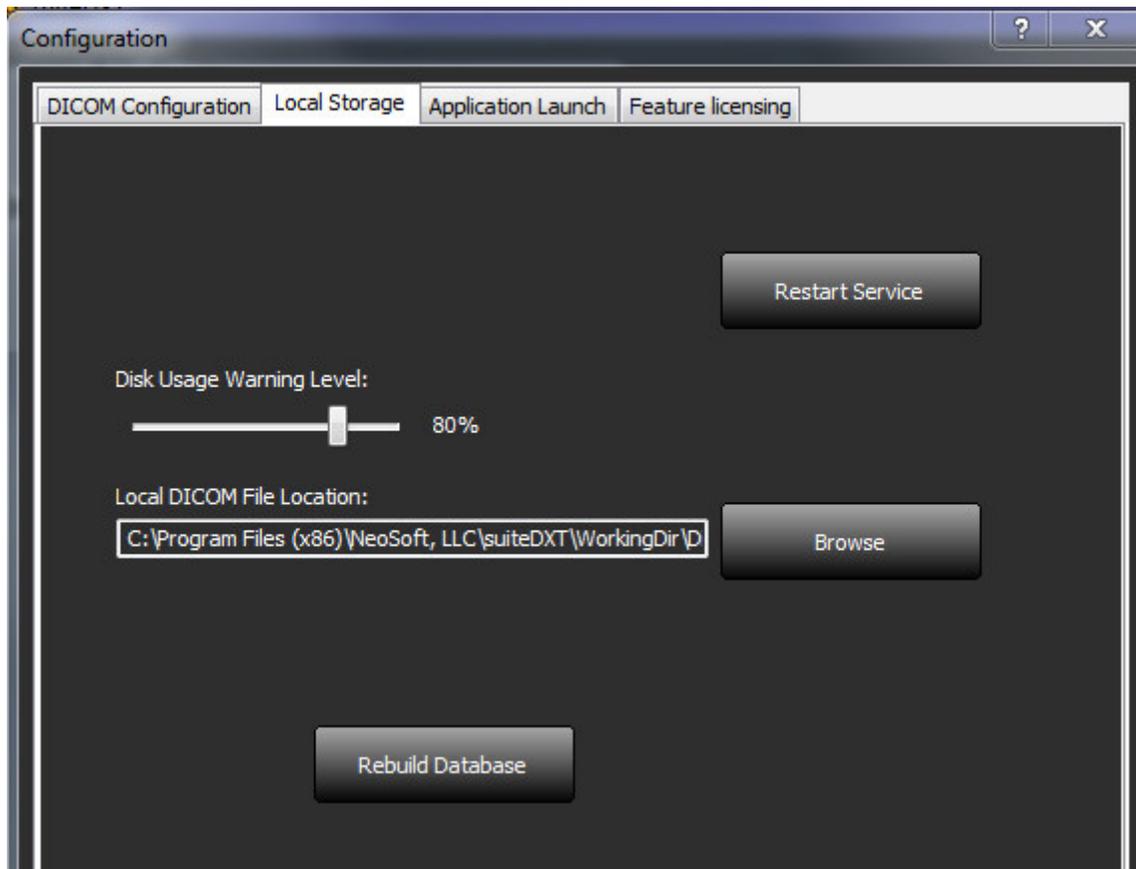

The Disk Usage Warning Level can be modified to alert you when disk space is low. When disk usage exceeds the limit set, the indicator on the main screen (Figure 6) will change from green to yellow.

To restore the study listing, click the Rebuild Database button. This refreshes the data currently stored on the local DICOM file location.

FIGURE 6. Disk Usage Indicator on Main Screen



The Local DICOM File Location Selection allows you to change the directory where DICOM data is stored. If data already exists in the location you've selected, it will be deleted before assigning a new folder. A warning message will appear to alert you to potential data loss.



CAUTION: Do not delete DICOM data from the file system.

Application Launch Tab

Use this tab to configure compatible NeoSoft, LLC applications to launch from suiteDXT.

1. Select the Add button (Figure 7) to open the Edit Application Window (Figure 8).

FIGURE 7. Application Launch Tab Window


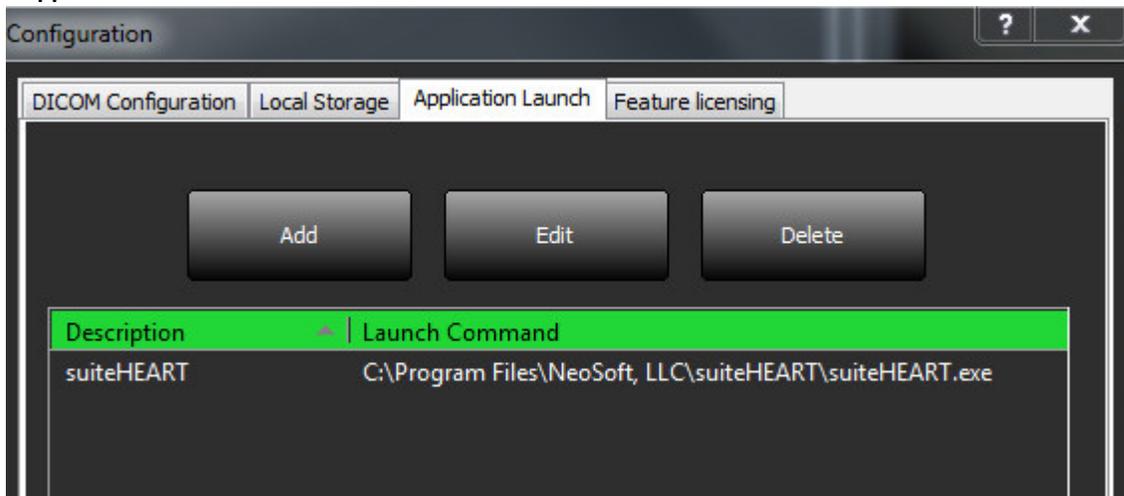


FIGURE 8. Edit Application Window

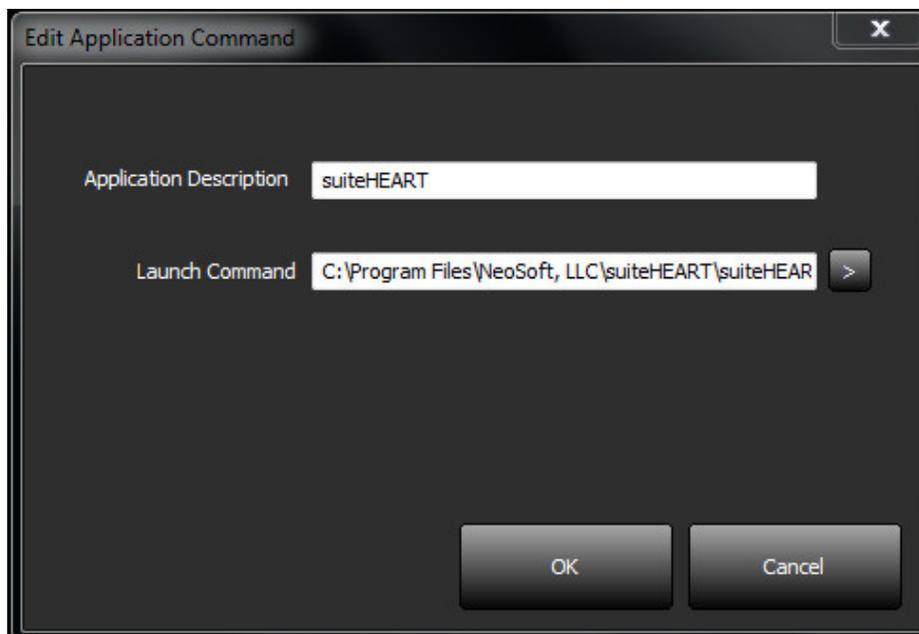

2. Enter the name or a description of the application.
3. Select the arrow button next to the Launch Command field to select the directory which contains the NeoSoft application executable file.
4. Select the OK button.

To edit or delete an existing application from the launch list, use the Edit or Delete button (Figure 7).

Feature Licensing Tab

Use this tab to request and apply the license for all software distributed by NeoSoft, LLC.

FIGURE 9. Feature Licensing Tab Window

The screenshot shows a software window titled "Feature licensing" with four tabs: "DICOM Configuration", "Local Storage", "Application Launch", and "Feature licensing". The window is divided into two main sections: "Request License" and "Apply License File".

Request License Section:

- Company Information:** Includes three input fields: "Name", "Telephone", and "Billing Address".
- Contact Information:** Includes three input fields: "First Name", "Last Name", and "Email".
- A "Generate License Request" button is located below the contact information fields.

Apply License File Section:

- An "Apply License" button is located within this section.

At the bottom right of the window are "OK" and "Cancel" buttons.

NOTE: Access to email will be needed to request a license.

Request a License

1. Enter complete company and contact information.

NOTE: Selecting the Generate License Request button will create a machine specific file that locks the software for which you are requesting a license, to the hardware (host) on which suiteDXT is installed.

2. Select the Generate License Request button.
3. Navigate to a memorable directory (e.g. the desktop) in which to save the license request file.
4. Email the license request file to licensing@neosoftmedical.com

Apply the License

1. From NeoSoft's response email, copy the license to an easily accessible location (e.g. the desktop).
2. Open suiteDXT, select the Configuration button and navigate to the Feature Licensing tab (Figure 9).
3. Select the Apply License button and navigate to the directory to which you saved the license.
4. Select OK.

Tablet Mode

suiteDXT is supported on tablets with a 64-bit processor running on Windows 10 Professional or Windows 10 Enterprise operating system.

To activate the keyboard click on the windows keyboard icon located in the lower right corner.

FIGURE 10. Keyboard



suiteHEART® Software Installation

Prerequisites

Prior to installation of the software, the following prerequisites must be met:

Table 1: System Requirements

Minimum System Requirements
Supported Operating Systems: <ul style="list-style-type: none">• Windows 7 Professional or Enterprise with SP1 (64 bit version)• Windows 10 Professional or Enterprise (64 bit version)
Video card (NVIDIA); 4GB RAM, minimum of 1664 CUDA Cores, support for OpenGL 4.0, support 1920 x 1080 resolution or higher
Monitor shall support 1920 x 1080 resolution or higher
Anti-Virus/Anti-Malware software installed
Minimum 16GB memory
Available hard drive space minimum 25GB
PDF viewer, Adobe Reader 11.0 or higher
An open network port for DICOM transfer over network
Static IP address (recommended)
Java Runtime Environment (JRE) version 8 (update 60 or later)
CUDA Toolkit version 8.0.61 or later
Solid-State hard drive
Intel® Core™ i7 processor
27" Monitor

NOTE: suiteHEART® Software is not supported in Virtual Machine environments.

NOTE: suiteHEART® Software does not support scaling/zoom levels greater than 125%.

NOTE: You must be logged into your operating system as Administrator in order to install the software.

NOTE: For support of application frame rates of 30FPS at display resolutions in the range of 2K/4K, the NVIDIA video card hardware must support a minimum of 1920 CUDA Cores

Installation

1. Double-click on the suiteHEART® Software windows application installer.

NOTE: Installing the software on a machine could result in a Open File - Security Warning indicating that the publisher could not be verified. Click Yes when asked if you are sure you want to run the software.

2. Select the appropriate language for your installation and click **OK**.

NOTE: If another version of the software is already installed on the system, a pop-up will ask permission to overwrite. Click “Yes” to continue with the installation.

3. In the “Welcome to suiteHEART® Software Setup Wizard window, click **Next**.
4. On the License Agreement Window, select “I accept the agreement” and click **Next**.
5. Browse to the directory in which to install the software or use the default directory (recommended). Click **Next**.
6. Click **Next** on the Ready to Install screen.
A progress bar will display.
7. Click **Finish** to complete the installation.

Application Inactivity Setting

The suiteHEART® Software application will automatically close, save all analysis for the study and remove the associated lock file when the application has been inactive for 60 minutes. To change this setting do the following:

Navigate to the C:\Program Files\NeoSoft, LLC\suiteHEART\resources\properties\product.properties file and change the values of SHIDLE_TIMER to the desired time out. Note that the time is in seconds.

Licensing Schemes

suiteHEART® Software has 3 different licensing schemes. They are Evaluation, Unlimited and Per-Case Pack Limited.

1. Evaluation: This is a time limited license which does not allow the saving of analysis results or exam approval. Evaluation Version will be indicated on the report footer and splash screens. If the approval of an exam is attempted a message will appear stating: Evaluation version: Analysis state will not be saved.
2. Unlimited: No restrictions on analysis and is not case-limited.
3. Per-Case Pack Limited: The software will use the unique study instance id to identify the number of cases analyzed against the Per-Case Pack that has been purchased.

Once 100% of the Per-Case Pack has been used the software will indicate this condition by a pop-message prior to starting a new exam or an existing exam.

Per-Case Packs can be purchased in increments of 25, 50 and 100. Website: <http://neosoftllc.com/> T: (262)522-6120
email: orders@neosoftmedical.com

Exams that have been counted once towards the Per-Case Pack limit can be re-opened and reviewed within the software and will not be counted against the Per-Case Pack limit.

Exams that are opened only for image viewing or if image manipulation tools are performed (Pan, Zoom, Window level, Rotate) will not be counted against the Per-Case Pack limit.

An exam is considered "consumed" or "counted" against the Per-Case Pack limit when any of the following actions are performed:

- a.) Starting of any analysis mode by placing any ROI on an image.
- b.) Creating a custom series.
- c.) Report sign off.
- d.) Export Cine DICOM.
- e.) Export Report.
- f.) DICOM Import.
- g.) Switching function analysis types.

suiteHEART® Software has an expected useful service life of 7 years from its original release date.

Remote Connectivity

Remote connectivity allows suiteHEART® Software users remote access from computers not loaded with suiteHEART® Software. The remote user will have the ability to access the suiteHEART® Software system and have full functionality.

suiteHEART® remote connectivity needs to be installed/configured/supported by your Information Technology personnel.

Remote connectivity has been verified using the following platforms:

- TeamViewer (version 11)
- Citrix GoToMyPC (version 8.4)
- Windows Remote Desktop (Microsoft Windows 7/8/10 Professional/Enterprise)

NOTE: When using Windows Remote Desktop, screen resolution on the remote computer must be set to 1920x1080 or higher video display resolution.

NOTE: When remotely accessing suiteHEART® Software using Windows Remote Desktop, the suiteHEART® 3D/4D viewer is not operational. The workaround is to use one of the other qualified remote access software packages (TeamViewer or GoToMyPC).

The performance of the suiteHEART® Software via the remote connection cannot be guaranteed. Performance is dependent upon factors that are outside the scope of the suiteHEART® Software application. These factors include:

- Remote computer performance
- Internet download/upload speeds (Mbps)
- Network bandwidth speed (wired ethernet or wireless connection)

For more information on remote connectivity, refer to the suiteHEART® Software Addendum to Instructions for Use manual, NS-03-015-0006.

This page intentionally left blank.